

## OPUS

12SXXXXX0



OPUS is the new generation of spectral sensors for online measurement of nitrogen and carbon compounds. Through the analysis of a full spectrum, OPUS is able to deliver reliable readings for  $\text{NO}_3\text{-N}$ ,  $\text{NO}_2\text{-N}$ , organic ingredients (CODeq, BODeq, DODeq, TOCeq), and a number of other parameters.

OPUS features the new TriOS G2 interface, allowing fast and easy configuration of sensors by using a web browser.

Integration into existing process control systems and external data loggers has never been easier.

With the optional battery pack, mobile applications are also feasible. WiFi connectivity allows laptops, tablets or smartphones to be easily used for control without any special application software or app installation.


### Benefits

- Without sampling and preparation of test samples
- Real-time sensor
- Without reagents
- Optical window with nano coating
- Pre-installed application calibration

### Applications

- Sewage treatment plants
- Environmental monitoring
- Drinking water monitoring
- Industrial applications

### Absorption spectrum of wastewater with/without CODeq

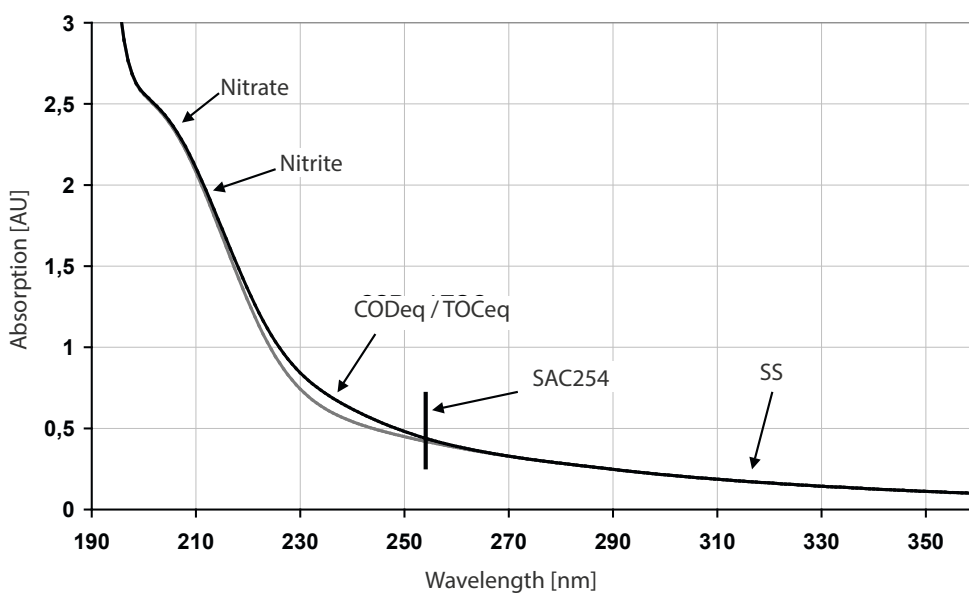

## Technical Specifications

<b>Measurement technology</b>	light source	Xenon flash lamp
	detector	High-end miniature spectrometer
		256 Channels
		200 to 360 nm
	0.8 nm/pixel	
<b>Measurement principle</b>		Attenuation, spectral analysis
<b>Optical path</b>		0.3 mm, 1 mm, 2 mm, 5 mm, 10 mm, 50 mm
<b>Parameter</b>		See parameter list
<b>Measuring range</b>		See parameter list
<b>Measurement accuracy</b>		See parameter list
<b>Turbidity compensation</b>		Yes
<b>Data logger</b>		~ 2 GB
<b>T100 response time</b>		2 min
<b>Measurement interval</b>		≥ 1 min
<b>Housing material</b>		Stainless steel (1.4571/1.4404) or titanium (3.7035)
<b>Dimensions (L x Ø)</b>		470 mm x 48 mm (with 10 mm path)
<b>Weight</b>	stainless steel	~ 3 kg (with 10 mm path)
	titanium	~ 2 kg (with 10 mm path)
<b>Interface</b>	digital	Ethernet (TCP/IP)
		RS-232 or RS-485 (Modbus RTU, ASCII, TriOS, (SCPI))
<b>Power consumption</b>		≤ 8 W
<b>Power supply</b>		12-24 VDC (± 10 %)
<b>Maintenance effort</b>		Typically ≤ 0.5 h/month
<b>Calibration/maintenance interval</b>		24 months
<b>System compatibility</b>		Modbus RTU
<b>Guarantee</b>		1 year (EU: 2 years)
<b>INSTALLATION</b>		
<b>Max. pressure</b>	with SubConn	30 bar
	with fixed cable	3 bar
	in FlowCell	1 bar, 2-4 L/min
<b>Protection type</b>		IP68
<b>Sample temperature</b>		+2...+40 °C
<b>Ambient temperature</b>		+2...+40 °C
<b>Storage temperature</b>		-20...+80 °C
<b>Inflow velocity</b>		0.1-10 m/s

## Measuring range

Single parameter under optimum laboratory conditions

Path (mm)	Parameter	Measurement principle	Unit	Measuring range	Detection limit	Limit of determination	Precision	Accuracy*
1	Nitrat NO <sub>3</sub> -N	Spectral	mg/L	0 - 100	0.3	0.5	0.05	± (5 % + 0.1)
	Nitrit NO <sub>2</sub> -N	Spectral	mg/L	0 - 150	0.5	1.2	0.12	± (5 % + 0.1)
	CODeq	Spectral	mg/L	0 - 2200***	30	100	10	
	BODeq	Spectral	mg/L	0 - 2200***	30	100	10	
	DOCeQ	Spectral	mg/L	0 - 1000	5	10	1	
	TOCeQ	Spectral	mg/L	0 - 1000	5	10	1	
	TSSeq	Spectral	mg/L	0 - 1500	60	200	20	
	KHP	Spectral	mg/L	0 - 4000	5	10	1	± (5 % + 2)
	SAC <sub>254</sub>	Single wavelength	1/m	0 - 2200	15	50	5	
	COD-SACeq**	Single wavelength	mg/L	0 - 3200	22	73	7.3	
	BOD-SACeq**	Single wavelength	mg/L	0 - 1050	7.2	24	2.4	
	10	Nitrat NO <sub>3</sub> -N	Spectral	mg/L	0 - 10	0.03	0.05	0.005
Nitrit NO <sub>2</sub> -N		Spectral	mg/L	0 - 15	0.05	0.12	0.012	± (5 % + 0.01)
CODeq		Spectral	mg/L	0 - 220***	3	10	1	
BODeq		Spectral	mg/L	0 - 220***	3	10	1	
DOCeQ		Spectral	mg/L	0 - 100	0.5	1	0.1	
TOCeQ		Spectral	mg/L	0 - 100	0.5	1	0.1	
TSSeq		Spectral	mg/L	0 - 150	6	20	2	
KHP		Spectral	mg/L	0 - 400	0.5	1	0.1	± (5 % + 0.2)
SAC <sub>254</sub>		Single wavelength	1/m	0 - 220	1.5	5	0.5	
COD-SACeq**		Single wavelength	mg/L	0 - 320	2.2	7.3	0.73	
BOD-SACeq**		Single wavelength	mg/L	0 - 105	0.72	2.4	0.24	

\* Based on a standard calibration solution

\*\* Based on KHP (100 mg COD standard solution correspond to 85 mg/L KHP)

\*\*\* Depending on composition of COD and BOD (checksum parameter)

1 mg/L NO<sub>3</sub>-N correspond to 4.43 mg/L NO<sub>3</sub>

1 mg/L NO<sub>2</sub>-N correspond to 3.29 mg/L NO<sub>2</sub>



## OPUS G2 interface

The easiest and fastest way of sensor integration and configuration in any process control system or data logger via web browser:

Let OPUS automatically monitor your processes and react to unexpected events or incidents with alerts: Thanks to the optional "policing" feature of OPUS.

